


Meas.Nr. 48999 **Date** Montag, 14 Mai 2012 04:45 **Personal Report No.:**
Material Yellow Paste 2 original sample **M120102**
Description dedisp. in EtOH; 30s ultrasonic LABORETTE 17

Calculation Fraunhofer broad **TradeOff** 1.000000e+002
Scans Fine 100 **Scans Coarse** 0 **Channels** 51 **Beam Obscuration** 20.00 %
Meas. Range 0.08 [µm] - 42.30 [µm] **Pump** 6

%	< µm
5.0	0.45
10.0	0.55
15.0	0.63
20.0	0.70
25.0	0.77
30.0	0.84
40.0	0.97
50.0	1.12
60.0	1.29
70.0	1.49
80.0	1.75
90.0	2.17
95.0	2.55
98.0	3.01
99.0	3.30

%	< µm
0.2	0.10
1.5	0.30
7.3	0.50
41.9	1.00
70.5	1.50
86.5	2.00
94.6	2.50
98.0	3.00
99.9	4.00
100.0	5.00
100.0	6.00
100.0	7.00
100.0	8.00
100.0	9.00
100.0	10.00

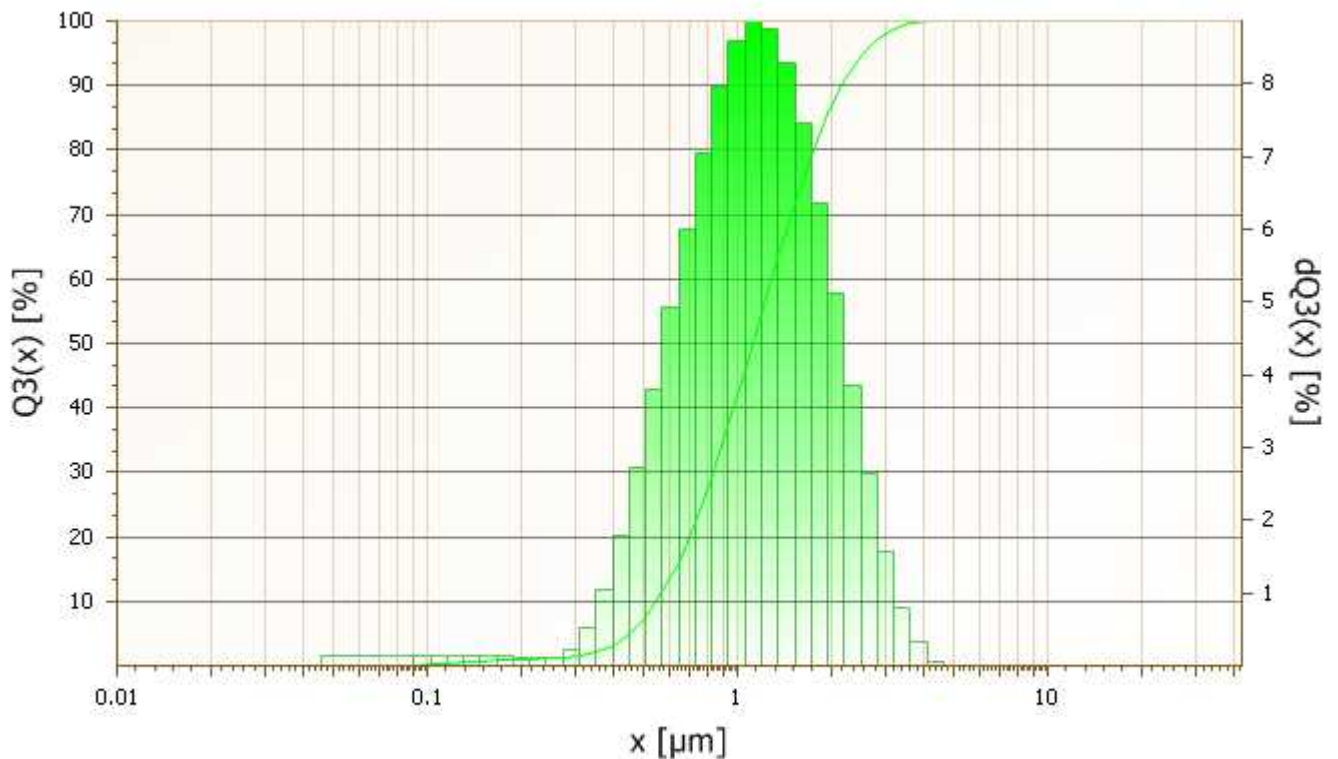

▲ 48999 dQ3(x) — 48999 Q3(x)