


Meas.Nr. 62042 **Date** 03.11.2013 11:55 **Personal Report No.:**
Material Silica 15min P5cl 250ml ZrO2 1mm **M130031**
Description predisp. with 0,1%Na4P2O7+ 1min ultrasonic LABORETTE 17

Calculation Mie n = 1.54 -i 0 **broad TradeOff** 1.000000e+002
Scans Fine 100 **Scans Coarse** 0 **Channels** 51 **Beam Obscuration** 14.00 %
Meas. Range 0.08 [µm] - 42.30 [µm] **Pump** 5 **Ultrasonics** 10

%	< µm
5	0.372
10	0.437
15	0.490
20	0.538
25	0.584
30	0.629
40	0.721
50	0.819
60	0.930
70	1.062
80	1.239
90	1.507
95	1.752
98	2.054
99	2.233

%	< µm
0.00	0.10
0.00	0.15
0.00	0.20
1.38	0.30
16.00	0.50
48.06	0.80
65.37	1.00
97.67	2.00
99.99	3.00
100.00	5.00

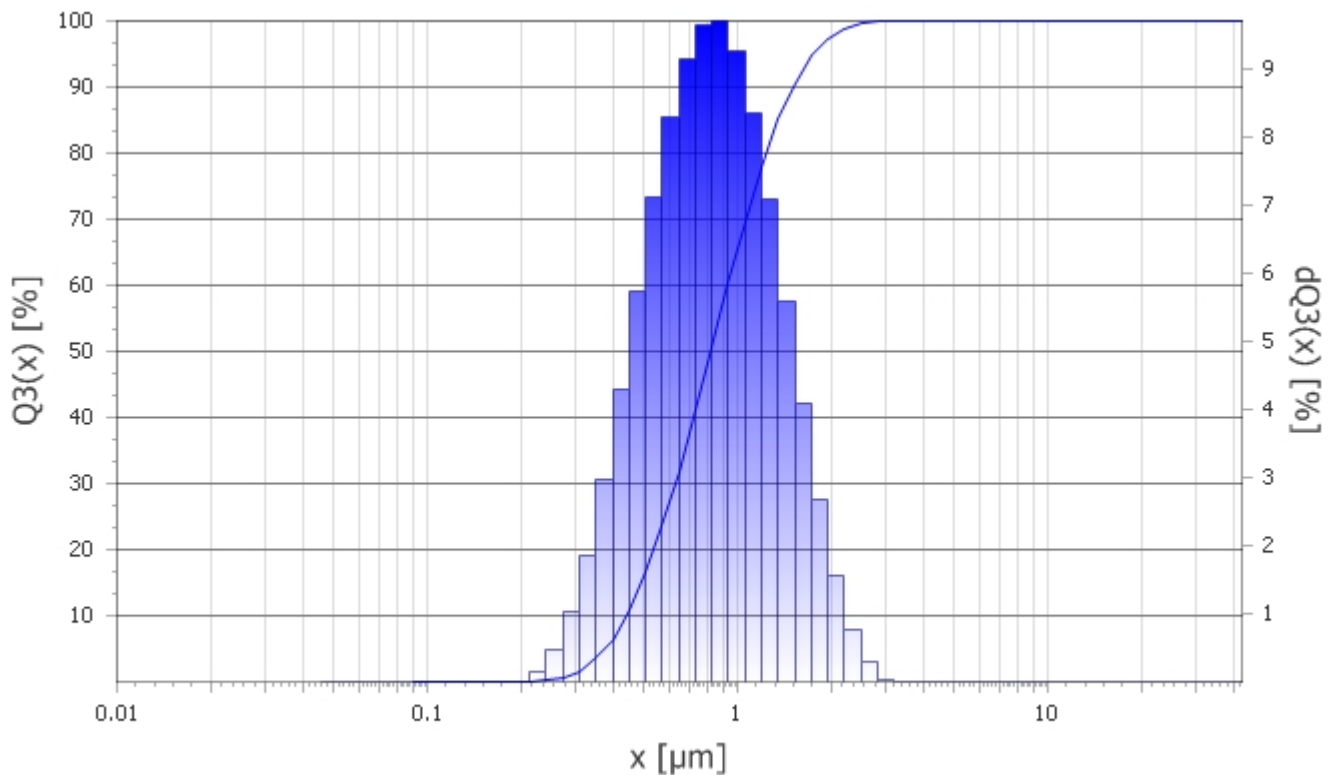

▲ 62042 dQ3(x) — 62042 Q3(x)