


**Meas.Nr.** 64732      **Date** Mittwoch, 29 Mai 2013 08:06      **Personal Report No.:**  
**Material** Exchange Resin Sample 2      60 min P6cl 5 mm steel      **M130074**  
**Description** predisp. 1min LABORETTE 17 ultrasonic

**Calculation** Fraunhofer      broad      **TradeOff** 1.000000e+003  
**Scans Fine** 100      **Scans Coarse** 100      **Channels** 102      **Beam Obscuration** 14.00 %  
**Meas. Range** 0.08 [µm] - 2000.00 [µm]      **Pump** 6      **Ultrasonics** 10

%	< µm
5	1.08
10	1.40
15	1.68
20	1.95
25	2.23
30	2.52
40	3.18
50	4.01
60	5.14
70	6.90
80	10.21
90	17.54
95	24.59
98	32.50
99	37.39

%	< µm
0.0	0.1
0.5	0.5
4.0	1.0
20.9	2.0
58.9	5.0
79.5	10.0
87.4	15.0
92.1	20.0
95.2	25.0
97.3	30.0
98.6	35.0
99.3	40.0
99.7	45.0
99.9	50.0
100.0	60.0

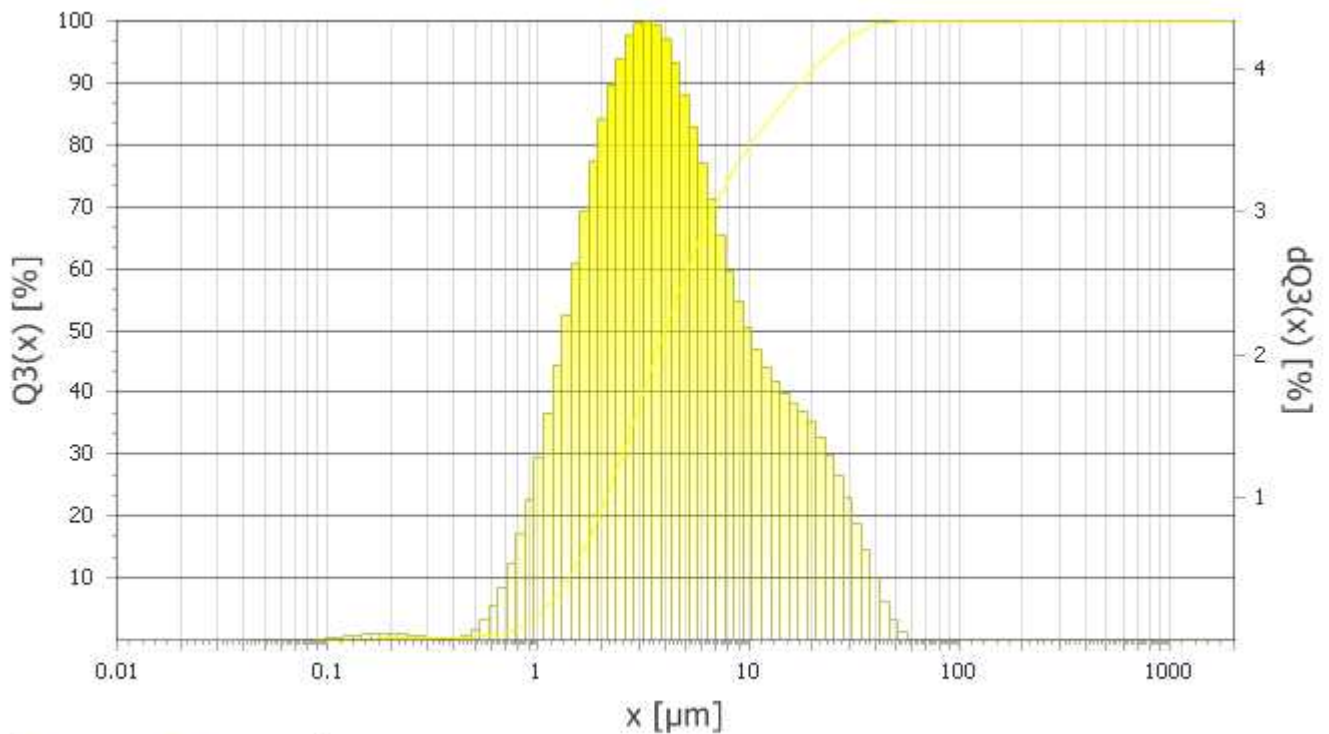

▲ 64732 dQ3(x)      — 64732 Q3(x)