


Meas.Nr. 63565 **Date** Freitag, 26 April 2013 11:20 **Personal Report No.:**
Material SiO2 dry 10 min P5cl 500ml ZrO2 5mm **M130103**
Description pre disp. in LABORETTE 17 ultrasonic bath - 1min in 0,1% Na4P2O7

Calculation Fraunhofer broad **TradeOff** 1.000000e+003
Scans Fine 100 **Scans Coarse** 100 **Channels** 102 **Beam Obscuration** 18.00 %
Meas. Range 0.08 [µm] - 2000.00 [µm] **Pump** 6 **Ultrasonics** 10

%	< µm
5	0.57
10	0.79
15	0.98
20	1.16
25	1.34
30	1.51
40	1.87
50	2.26
60	2.74
70	3.35
80	4.28
90	7.83
95	14.70
98	19.40
99	22.01

%	< µm
0.0	0.1
3.7	0.5
15.5	1.0
43.4	2.0
64.7	3.0
77.6	4.0
87.7	6.0
90.1	8.0
91.4	10.0
92.8	12.0
95.2	15.0
98.3	20.0
100.0	30.0
100.0	40.0

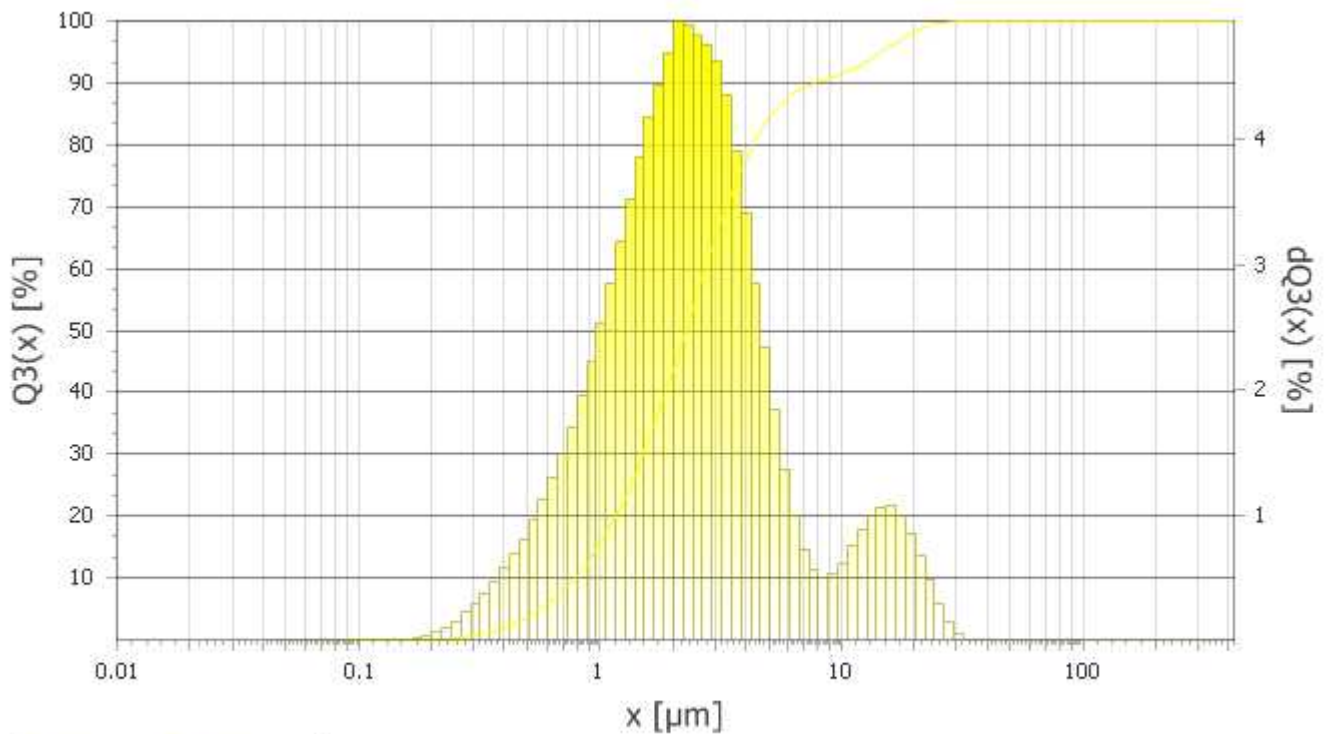

▲ 63565 dQ3(x) — 63565 Q3(x)