


Meas.Nr. 63561 **Date** Freitag, 26 April 2013 10:05 **Personal Report No.:**
Material SiO2 5min dry P5cl 500ml ZrO2 5mm **M130103**
Description directly dispersed in 0,1% Na4P2O7

Calculation Fraunhofer broad **TradeOff** 1.000000e+003
Scans Fine 100 **Scans Coarse** 100 **Channels** 102 **Beam Obscuration** 17.00 %
Meas. Range 0.08 [µm] - 2000.00 [µm] **Pump** 6 **Ultrasonics** 10

%	< µm
5	0.63
10	0.88
15	1.09
20	1.30
25	1.51
30	1.73
40	2.22
50	2.87
60	3.81
70	5.42
80	8.28
90	12.98
95	17.03
98	21.63
99	24.51

%	< µm
0.1	0.10
3.0	0.50
12.8	1.00
35.7	2.00
51.6	3.00
61.5	4.00
72.5	6.00
79.2	8.00
84.3	10.00
88.3	12.00
92.8	15.00
97.2	20.00
99.8	30.00
100.0	40.00

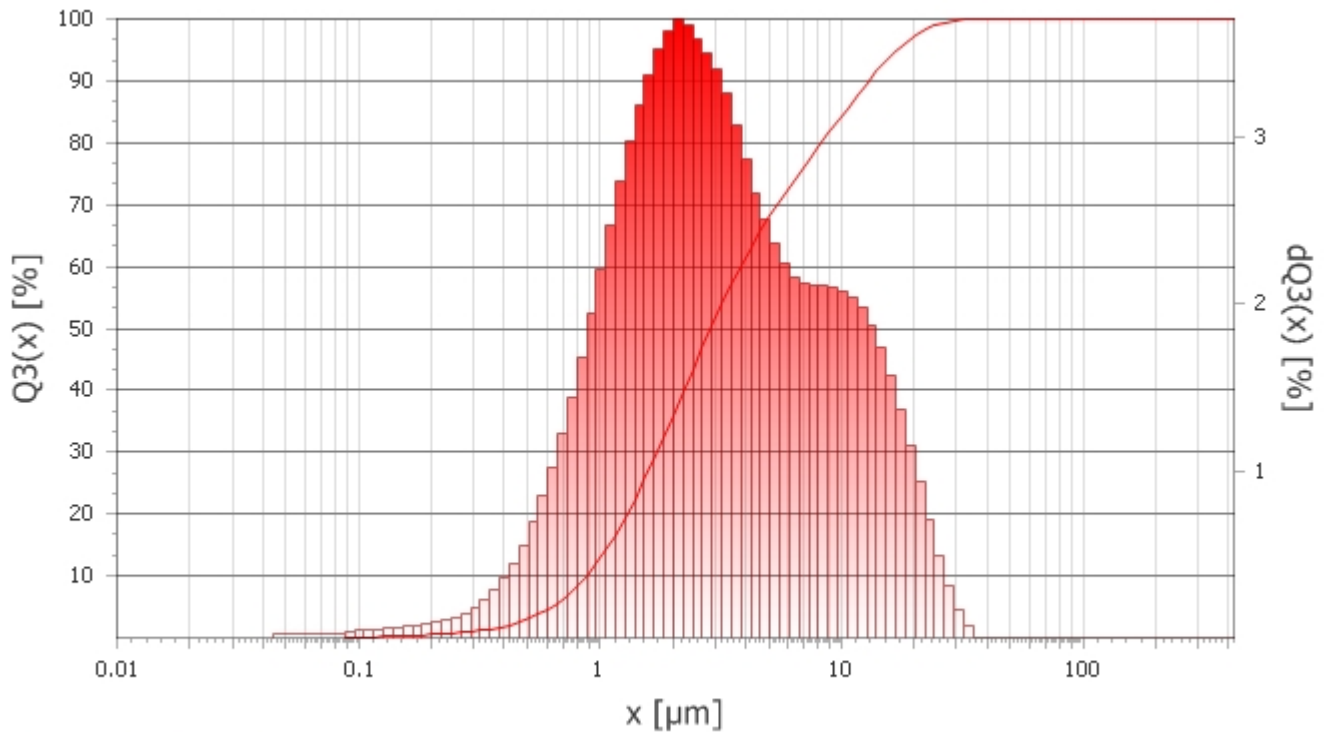

▲ 63561 dQ3(x) — 63561 Q3(x)