


Meas.Nr. 65110 **Date** Donnerstag, 13 Juni 2013 08:40 **Personal Report No.:**
Material Sprulina pwd. 30 min P7pl 2mm ZrO2 in water **M130134**
Description predisp. in 0,1% Na4P2O7 with 1min ultrasound LABORETTE 17

Calculation Fraunhofer broad **TradeOff** 1.000000e+002
Scans Fine 100 **Scans Coarse** 0 **Channels** 51 **Beam Obscuration** 12.00 %
Meas. Range 0.08 [µm] - 42.30 [µm] **Pump** 4 **Ultrasonics** 10

%	< µm
5	0.23
10	0.29
15	0.34
20	0.38
25	0.43
30	0.48
40	0.60
50	0.73
60	0.91
70	1.15
80	1.51
90	2.25
95	3.40
98	8.73
99	11.42

%	< µm
0.1	0.1
31.6	0.5
64.2	1.0
79.7	1.5
87.5	2.0
94.0	3.0
95.9	4.0
96.5	5.0
96.9	6.0
97.3	7.0
97.7	8.0
98.5	10.0
99.2	12.0
99.7	15.0
100.0	22.0

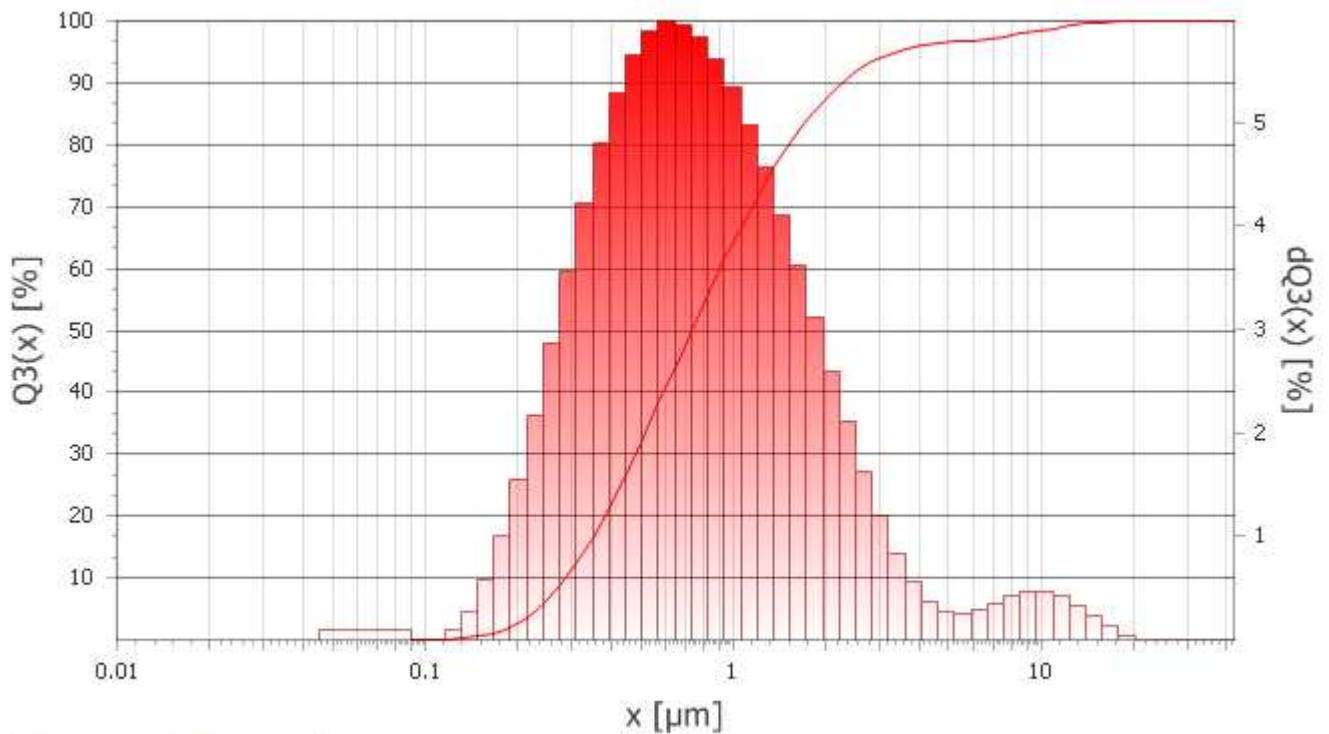

▲ 65110 dQ3(x) — 65110 Q3(x)