


Meas.Nr. 65348 **Date** 06.25.2013 09:13 **Personal Report No.:**
Material BaTiO₃ 15min P7pl 2mm ZrO₂ in water **M130162**
Description 0,1% Na₄P₂O₇ + 3min ultrasonic Laborette 17

Calculation Mie n = 1.6 -i 0 **broad TradeOff** 1.000000e+002
Scans Fine 100 **Scans Coarse** 0 **Channels** 108 **Beam Obscuration** 12.00 %
Meas. Range 0.01 [µm] - 42.30 [µm] **Pump** 4 **Ultrasonics** 10

%	< µm
5	0.056
10	0.073
15	0.084
20	0.094
25	0.103
30	0.112
40	0.131
50	0.150
60	0.173
70	0.202
80	0.241
90	0.309
95	0.391
98	1.106
99	1.574

%	< µm
1.97	0.02
3.34	0.03
4.13	0.05
13.03	0.08
23.29	0.10
49.86	0.15
69.45	0.20
89.10	0.30
96.83	0.50
97.26	0.80
97.72	1.00
99.50	2.00
99.94	3.00
100.00	5.00

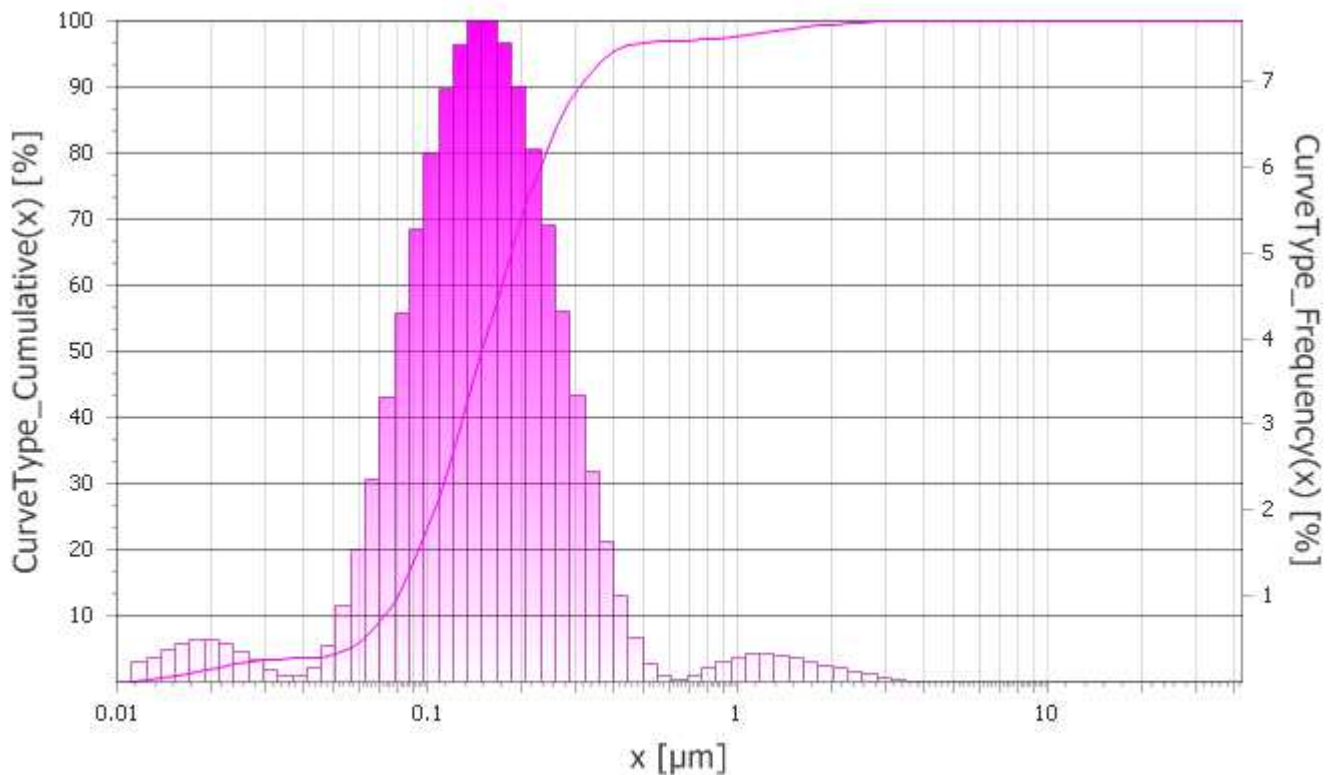

▲ 65348 dQ3(x) — 65348 Q3(x)