


Meas.Nr. 71200 **Date** 12.09.2013 08:31 **Personal Report No.:**
Material Asbestos 180 min P7pl 0,1 mm ZrO2 in water **M130287**
Description in water + 0,1 % Na4P2O7 - 1 min Ultrasonic LABORETTE 17

Calculation Mie n = 1.65 -i 0 **broad TradeOff** 1.000000e+002
Scans Fine 100 **Scans Coarse** 0 **Channels** 108 **Beam Obscuration** 4.00 %
Meas. Range 0.01 [µm] - 42.30 [µm] **Pump** 3 **Ultrasonics** 10

%	< µm
5	0.048
10	0.063
15	0.072
20	0.079
25	0.086
30	0.093
40	0.107
50	0.122
60	0.138
70	0.158
80	0.183
90	0.223
95	0.258
98	0.302
99	0.330

%	< µm
2.37	0.02
3.85	0.03
4.14	0.04
5.45	0.05
8.82	0.06
13.94	0.07
20.45	0.08
27.60	0.09
34.93	0.10
66.51	0.15
84.92	0.20
97.92	0.30
99.91	0.40
100.00	0.50

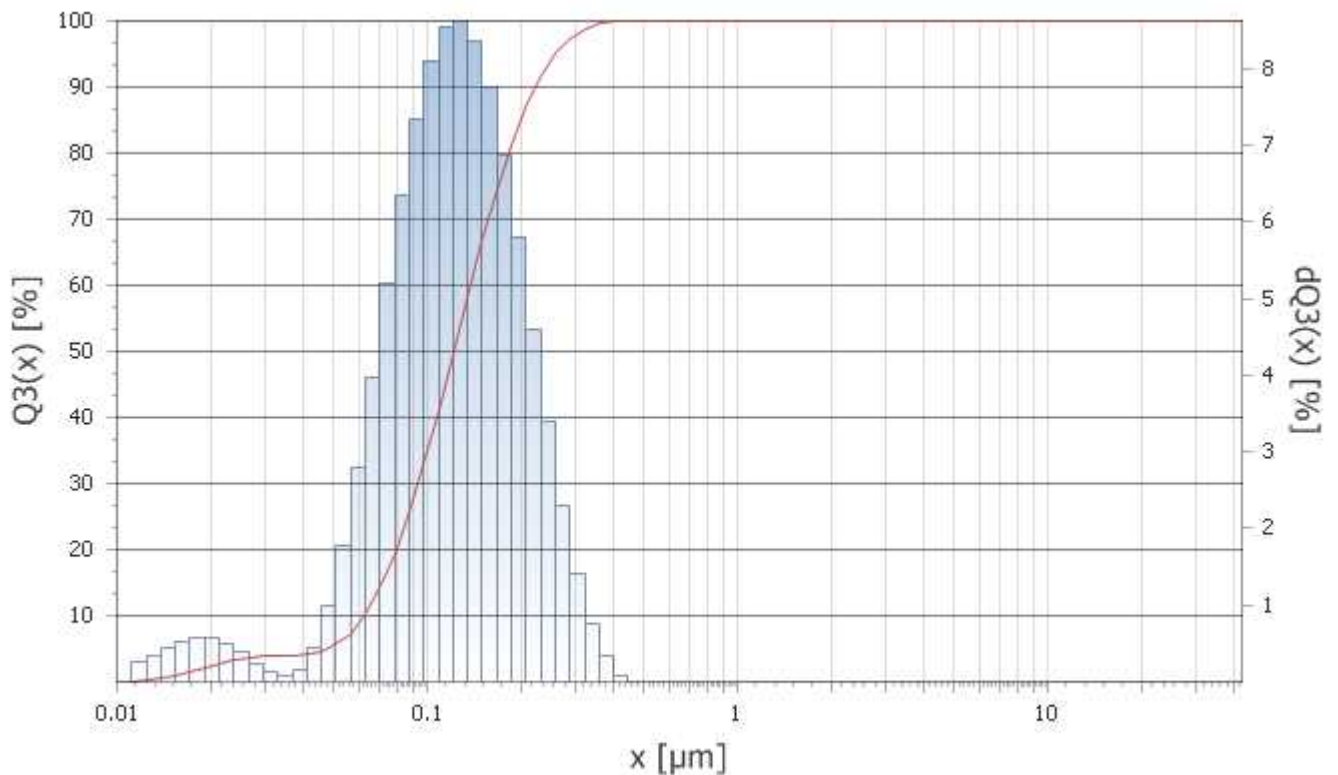

▲ 71200 dQ3(x) — 71200 Q3(x)