


Mess.-Nr.	71171	Datum	Friday, 06 December 2013 09:21 AM	Bearbeitungs- Nr.:	
Material	Diatomite		15 min P5 5 mm ZrO2	M130303	
Bemerkung	vordisp. in 0,1 % Na4P2O7, 1 min Ultraschall				

Berechnung	Fraunhofer	broad	TradeOff	1.000000e+003		
Scans	100	Scans	100	Messkanäle	108	
Feinbereich		Grobbereich		Strahlabsorption	12.00 %	
Messbereich	0,01	- 2000.00 [µm]	Pumpe	6	Ultraschall	10

%	< µm
5	0.45
10	0.65
15	0.80
20	0.94
25	1.07
30	1.20
40	1.48
50	1.79
60	2.15
70	2.61
80	3.29
90	4.56
95	6.21
98	9.41
99	11.83

%	< µm
1.2	0.1
6.1	0.5
22.4	1.0
40.7	1.5
56.1	2.0
76.3	3.0
86.7	4.0
91.9	5.0
94.6	6.0
96.2	7.0
97.1	8.0
98.3	10.0
99.1	12.0
99.7	15.0
100.0	20.0

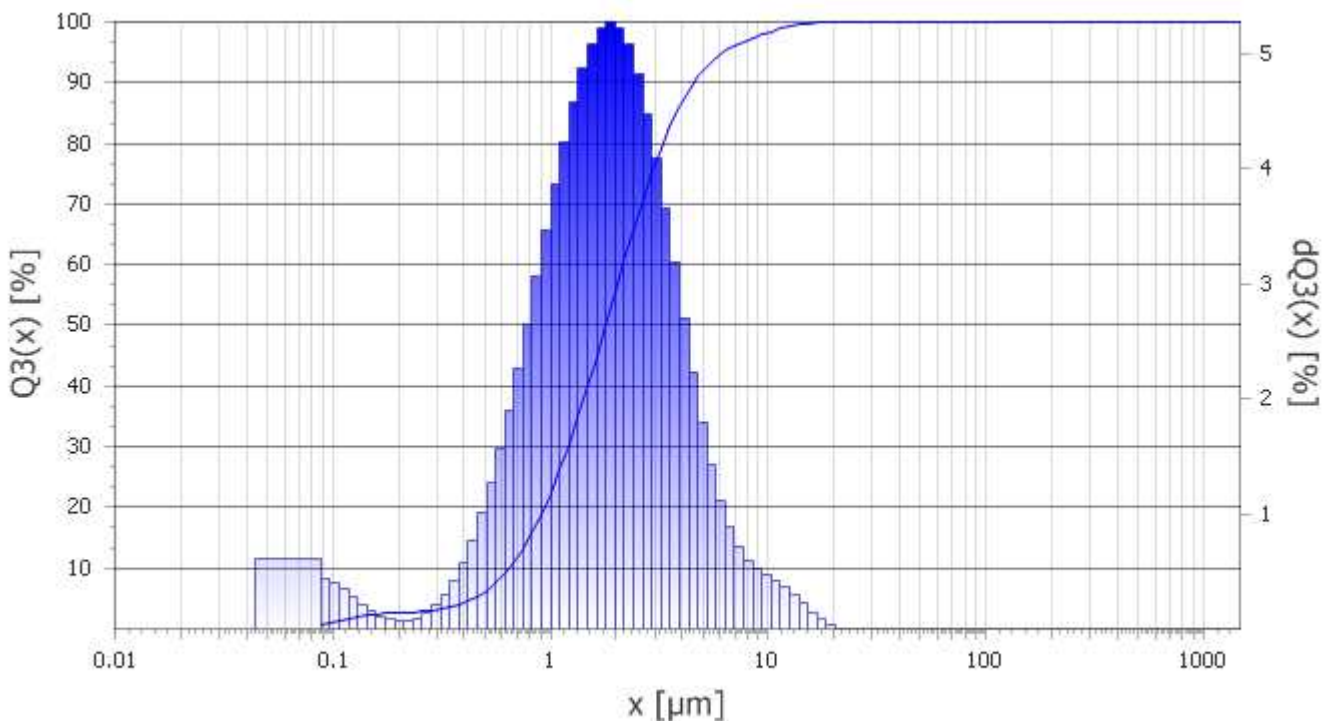

▲ 71171 dQ3(x) — 71171 Q3(x)