


ANALYSETTE 22 NanoTec plus

Meas.Nr. 71726 **Date** 01/06/2014 13:52 **Personal Report No.:**
Material Zirconium oxide 90min P7pl 0,5 mm ZrO2 **M130307**
Description predisp. in 0,1 % Na4P2O7 - 2 min Ultrasonic Bath LABORETTE 17

Calculation Mie n = 2.15130 -i 0 **broad TradeOff** 1.000000e+002
Scans Fine 100 **Scans Coarse** 0 **Channels** 108 **Beam Obscuration** 10.00 %
Meas. Range 0.01 [µm] - 42.30 [µm] **Pump** 3 **Ultrasonics** 10

%	< µm
5	0.011
10	0.017
15	0.031
20	0.037
25	0.041
30	0.046
40	0.054
50	0.063
60	0.073
70	0.086
80	0.105
90	0.153
95	0.385
98	0.501
99	0.568

%	< µm
4.45	0.01
10.38	0.02
13.97	0.03
35.35	0.05
65.67	0.08
77.75	0.10
91.63	0.20
92.70	0.30
95.46	0.40
97.99	0.50
99.32	0.60
99.83	0.70
99.96	0.80
99.98	0.90
99.98	1.00

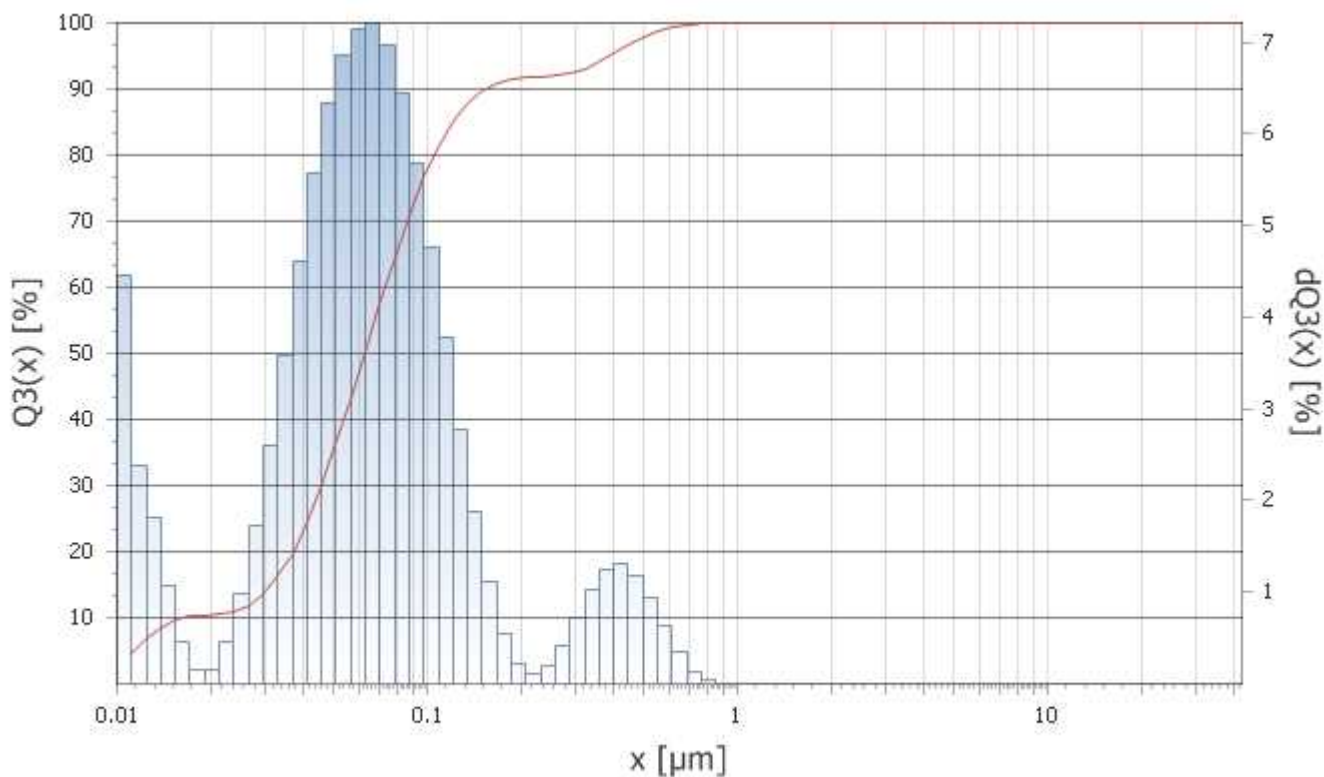

▲ 71726 dQ3(x) — 71726 Q3(x)