


Meas.Nr. 71717 **Date** Monday, 06 January 2014 11:25 AM **Personal Report No.:**
Material Porcelain 45min P5 350rpm 5mm ZrO2 **M130348**
Description predisp. 0,1 % Na4P2O7 water. 1 min ultrasound LABORETTE 17

Calculation Fraunhofer broad **TradeOff** 1.000000e+003
Scans Fine 100 **Scans Coarse** 100 **Channels** 102 **Beam Obscuration** 16.00 %
Meas. Range 0.08 [µm] - 2000.00 [µm] **Pump** 7 **Ultrasonics** 10

%	< µm
5	0.43
10	0.57
15	0.70
20	0.82
25	0.94
30	1.07
40	1.36
50	1.72
60	2.20
70	2.95
80	4.46
90	9.40
95	14.01
98	18.45
99	21.28

%	< µm
27.4	1.00
56.3	2.00
74.8	3.50
82.0	5.00
85.7	6.50
88.1	8.00
90.7	10.00
93.6	12.50
95.8	15.00
97.5	17.50
98.6	20.00
99.3	22.50
99.7	25.00
99.9	27.50
100.0	30.00

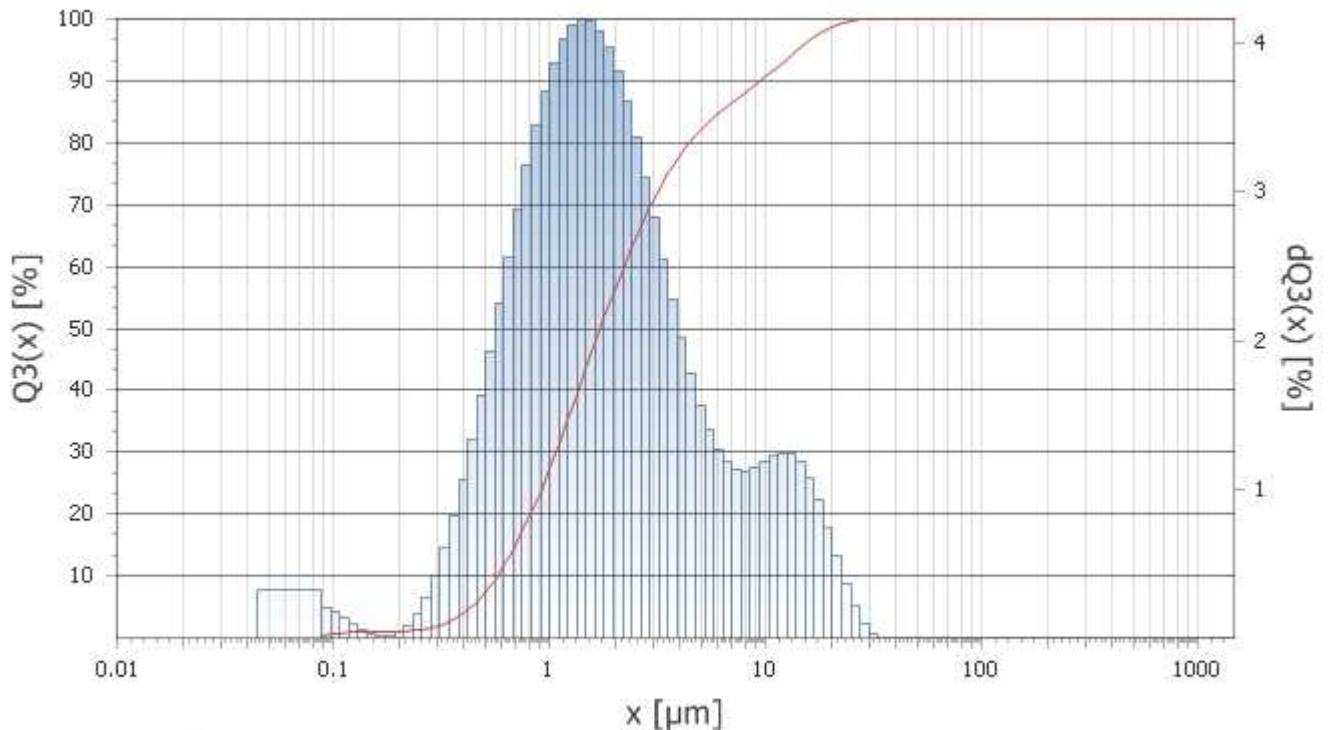

▲ 71717 dQ3(x) — 71717 Q3(x)