


Meas.Nr. 62244 **Date** Donnerstag, 14 März 2013 04:13 **Personal Report No.:**
Material Cement (in IPA) 15min P6cl 250ml WC 20mm **M130049**
Description predisp. in water with 0,1% Na₄P₂O₇ 1min ultrasonic LABORETTE 17

Calculation Fraunhofer broad **TradeOff** 1.000000e+003
Scans Fine 100 **Scans Coarse** 100 **Channels** 102 **Beam Obscuration** 14.00 %
Meas. Range 0.08 [µm] - 2000.00 [µm] **Pump** 8 **Ultrasonics** 10

%	< µm
5	0.66
10	1.01
15	1.39
20	1.83
25	2.39
30	3.12
40	5.49
50	9.30
60	14.04
70	19.51
80	26.10
90	35.31
95	42.75
98	50.87
99	56.14

%	< µm
0.0	0.1
2.7	0.5
9.9	1.0
38.4	5.0
51.6	10.0
61.9	15.0
70.8	20.0
78.5	25.0
84.8	30.0
89.8	35.0
93.4	40.0
97.7	50.0
99.4	60.0
99.9	70.0
100.0	80.0

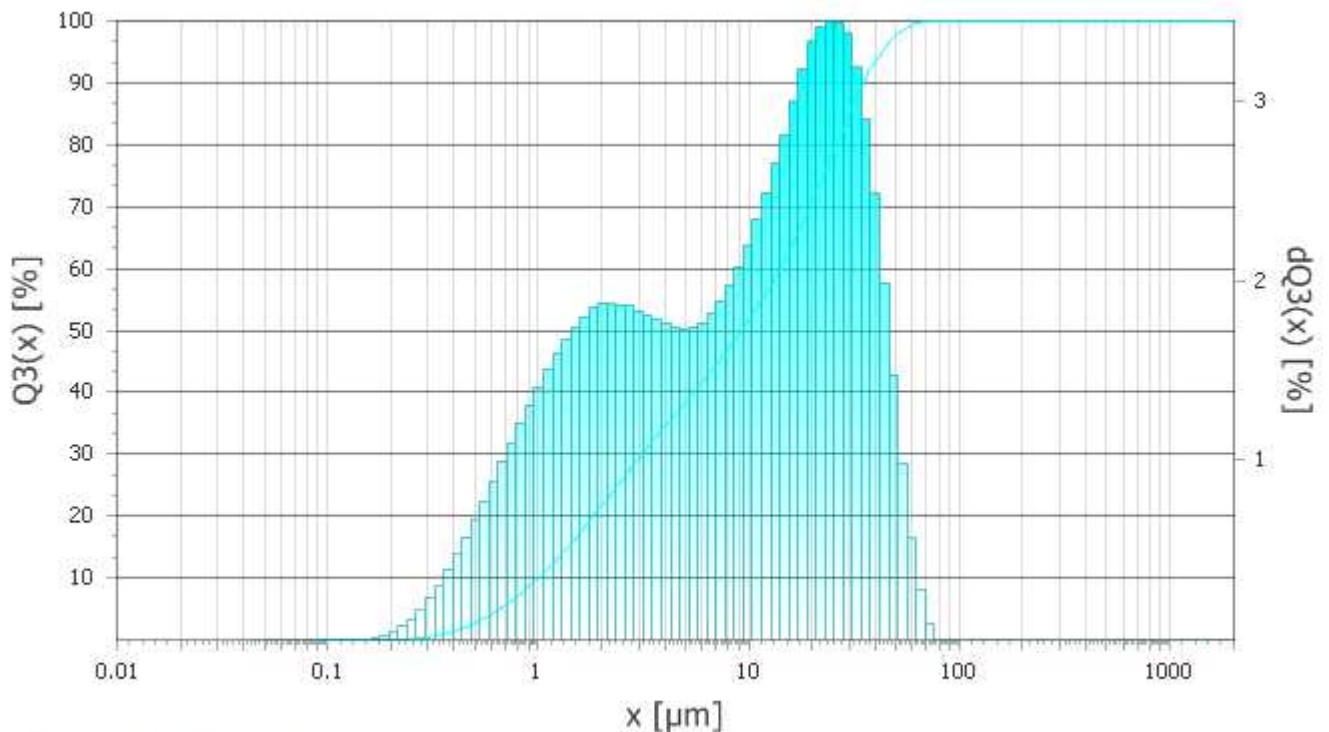

▲ 62244 dQ3(x) — 62244 Q3(x)